



STEP DOWN ICU PATIENT BED

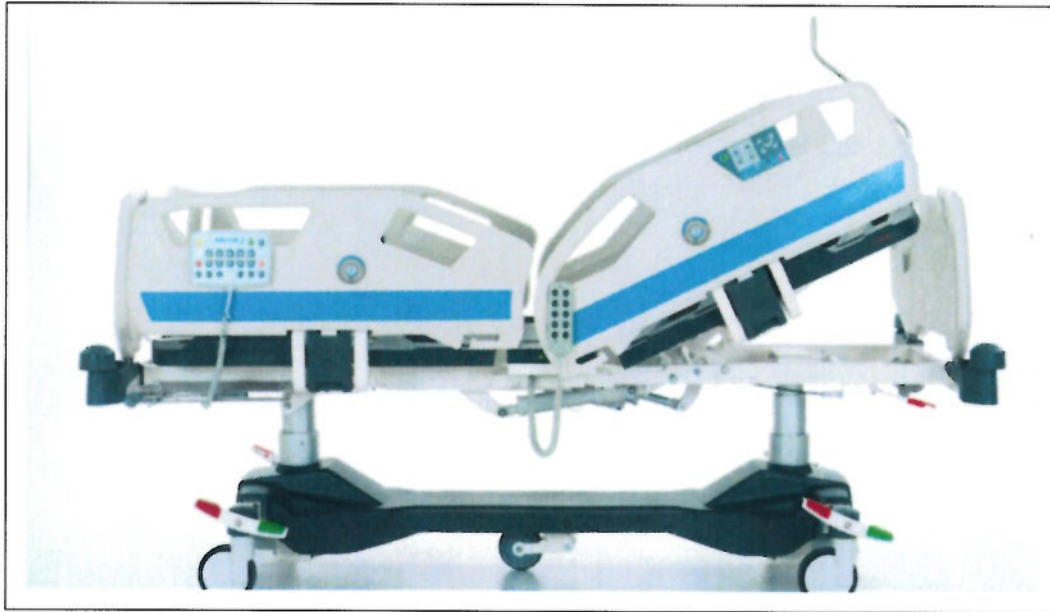

SPECIFICATIONS / REQUIREMENTS

1. Headrest, leg rest, height, Trendelenburg / reverse Trendelenburg adjustment
2. Fowler and Vascular position
3. With weighing scale system
4. Lateral position, column type (motor) - optional
5. Side rails control (nurse & patient), Nurse control panel can lock the functions
6. Bed extension.
7. Central locking system and 5th castor
8. IV pole, Oxygen cylinder (E-size) holder.
9. Weight capacity minimum 250 kg.
10. Mattress 150 mm thickness
11. Lifting pole, under bed light, x-ray cassette holder - optional
12. Mattress 150 mm thickness

PATIENT BED

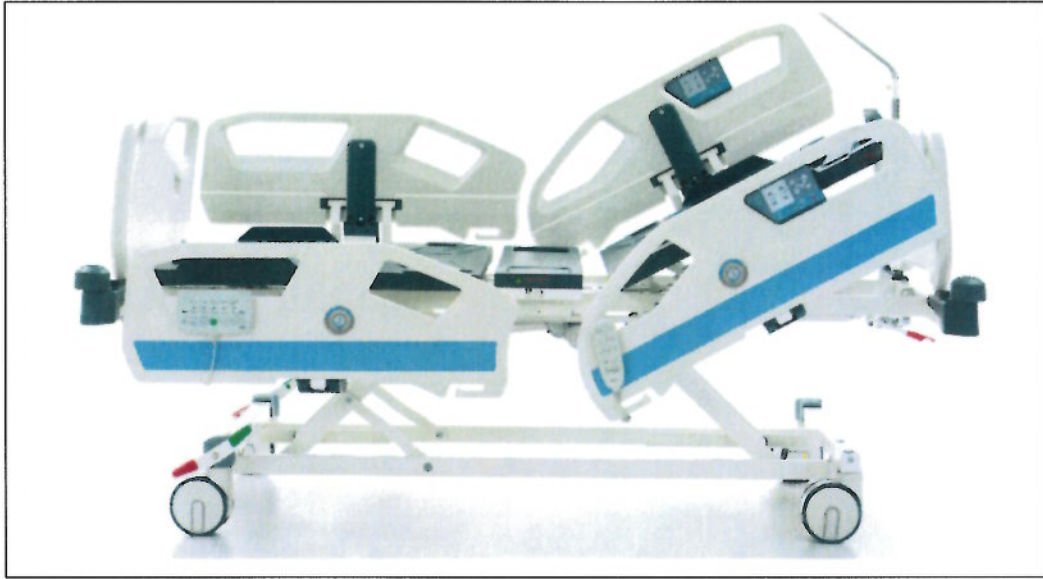

SPECIFICATIONS / REQUIREMENTS

1. Headrest, leg rest, height, Trendelenburg / reverse Trendelenburg adjustment
2. Fowler and Vascular position
3. 4 motors bed
4. Side rails control (nurse & patient), Nurse control panel can lock the functions
5. Bed extension.
6. Central locking system and 5th castor
7. IV pole, Oxygen cylinder (E-size) holder.
8. Weight capacity minimum 250 kg.
9. Mattress 150 mm thickness
10. Mattress 150 mm thickness